



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588

Atty Docket: DEXCOM.8DVC1

1/10

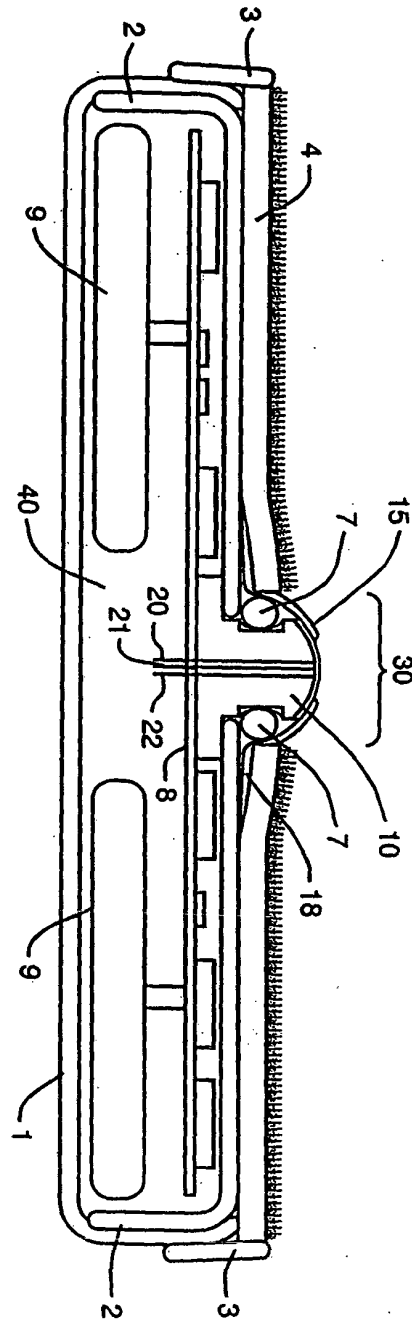


FIG. 1A



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588

Atty Docket: DEXCOM.8DVC1

2/10

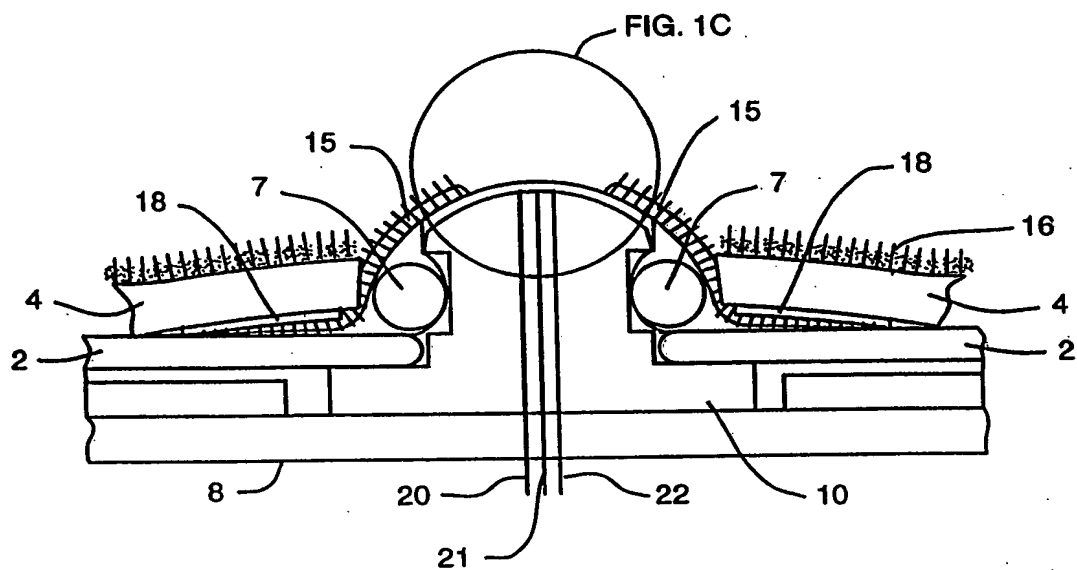


FIG. 1B

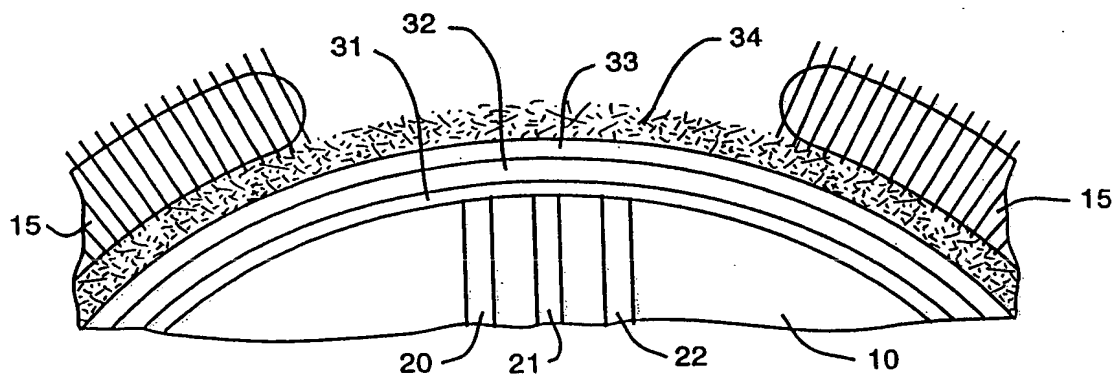


FIG. 1C



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588 Atty Docket: DEXCOM.8DVC1

3/10

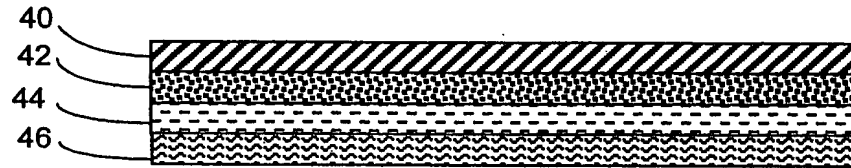


FIG. 1D



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588 Atty Docket: DEXCOM.8DVC1

4/10

SENSOR
GLUCOSE/MM

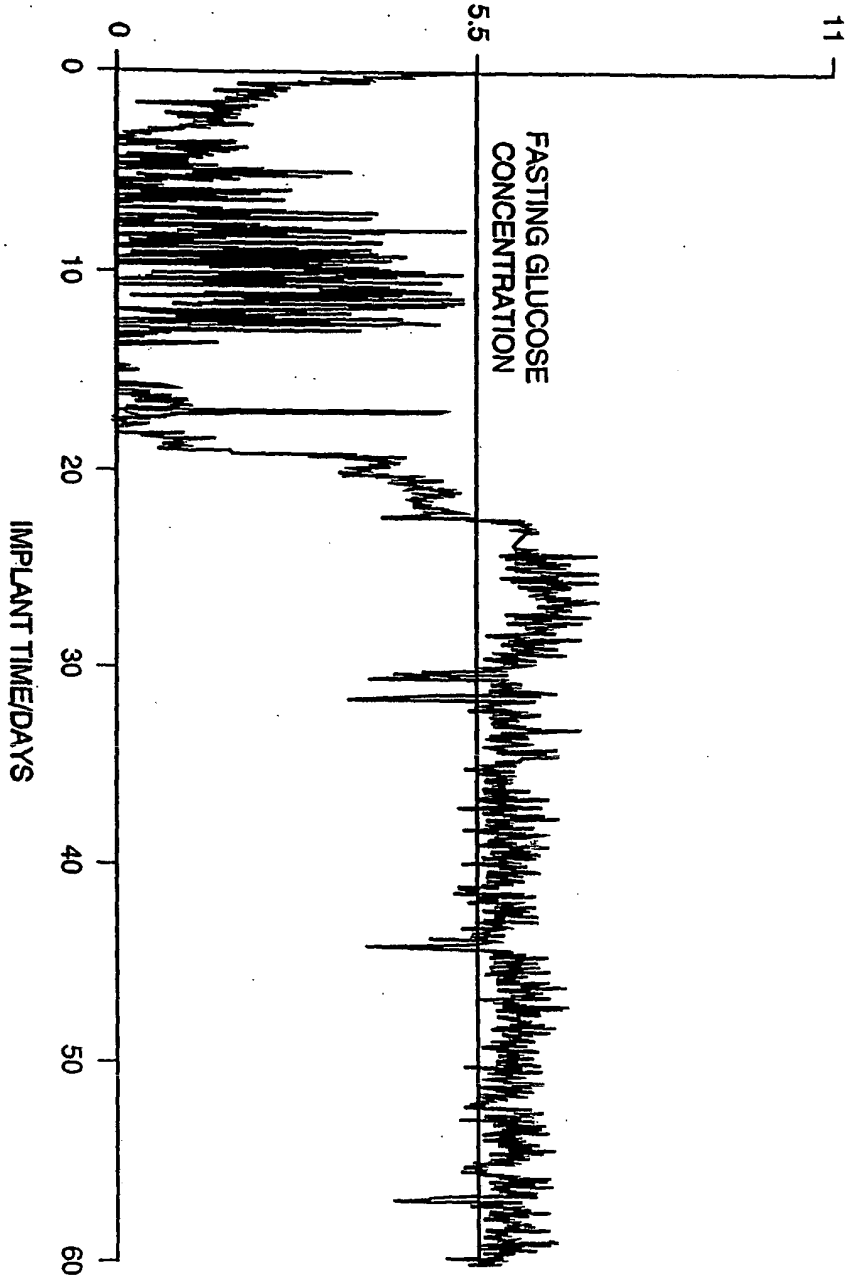


FIG. 2



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588

Atty Docket: DEXCOM.8DVC1

5/10

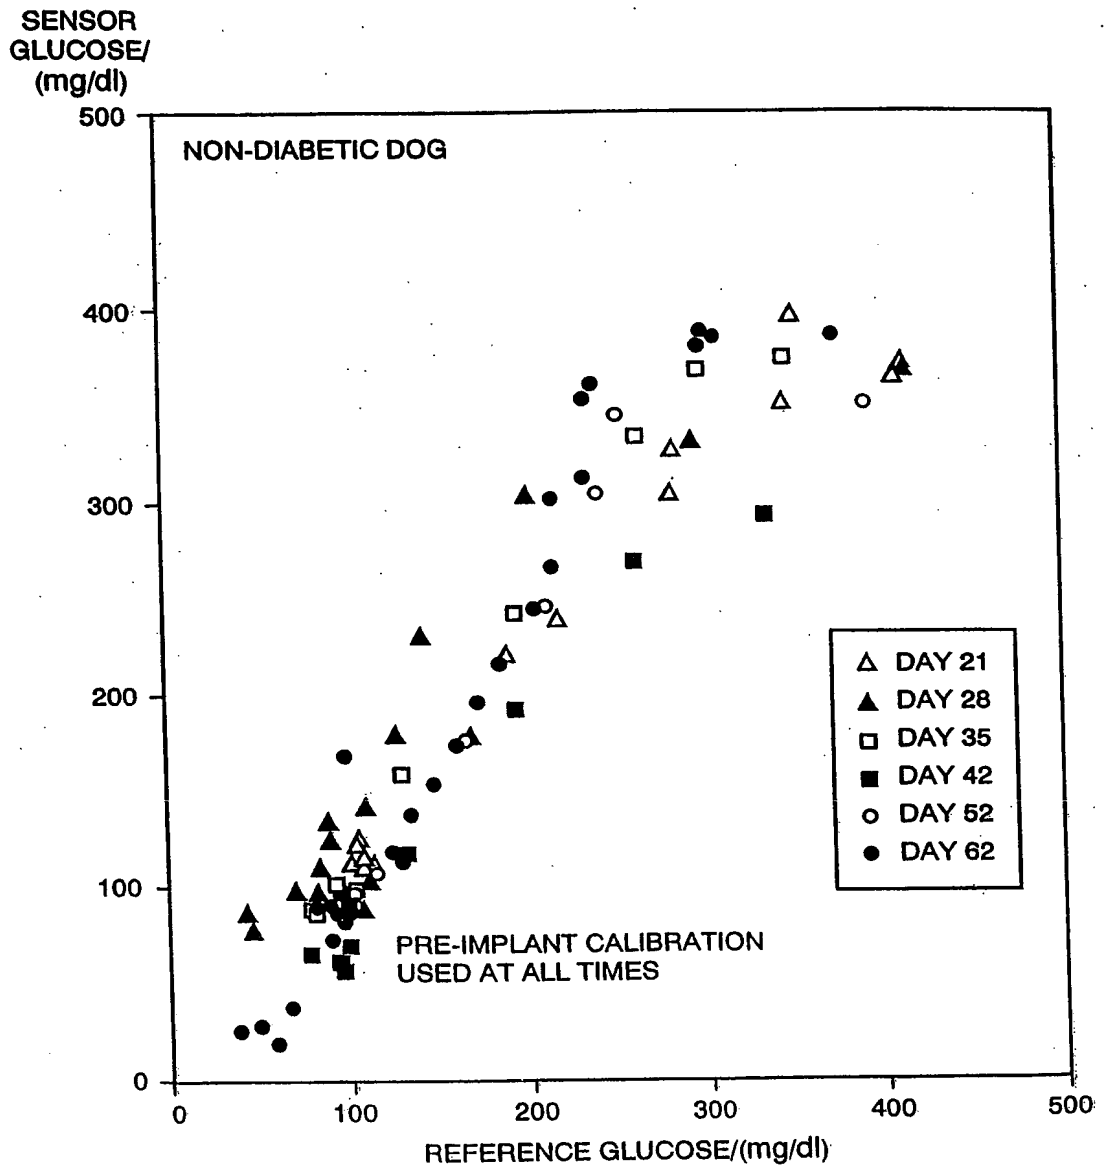


FIG. 3



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588

Atty Docket: DEXCOM.8DVC1

6/10

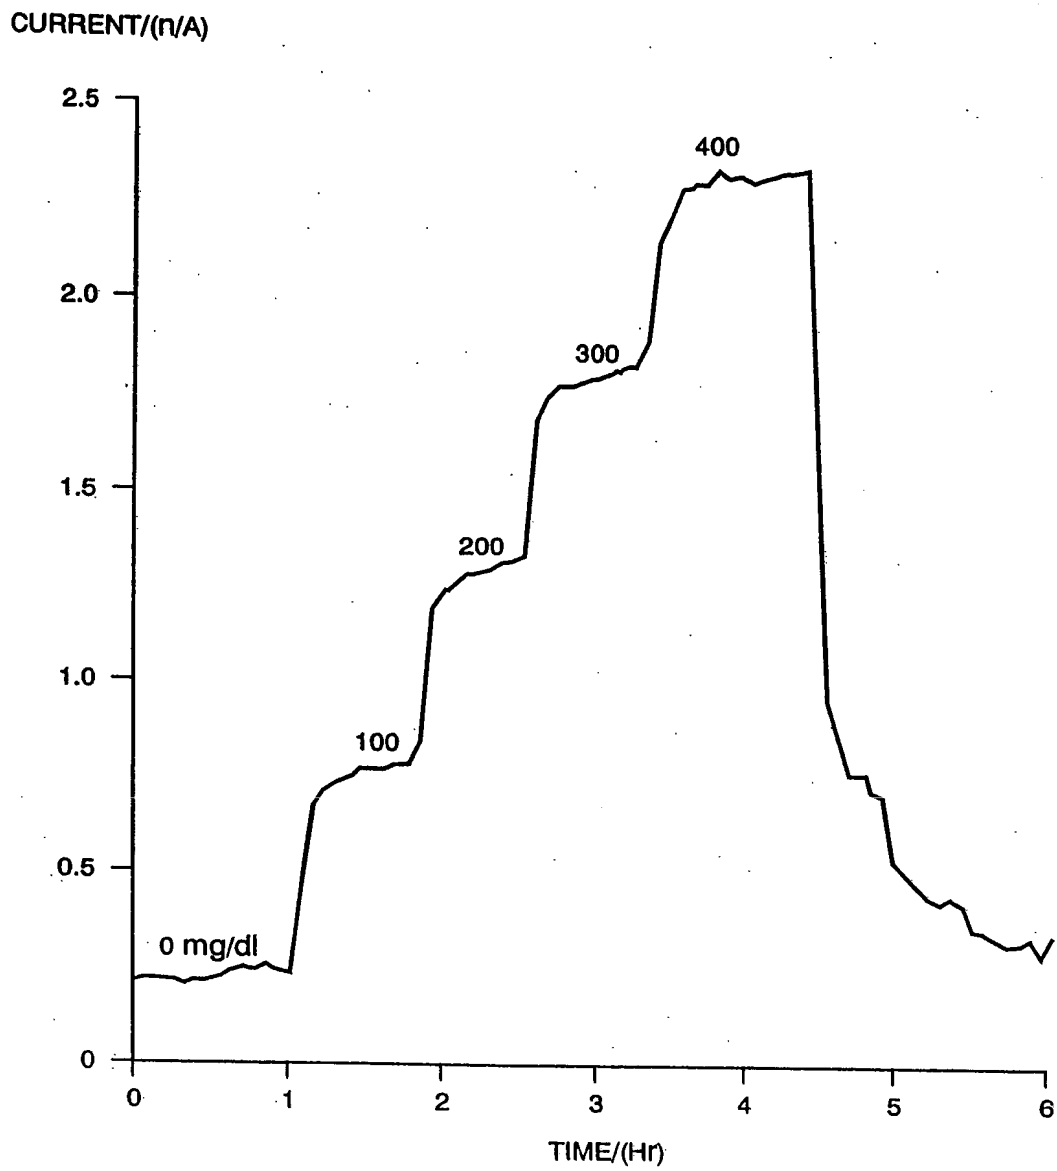


FIG. 4



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588 Atty Docket: DEXCOM.8DVC1

7/10

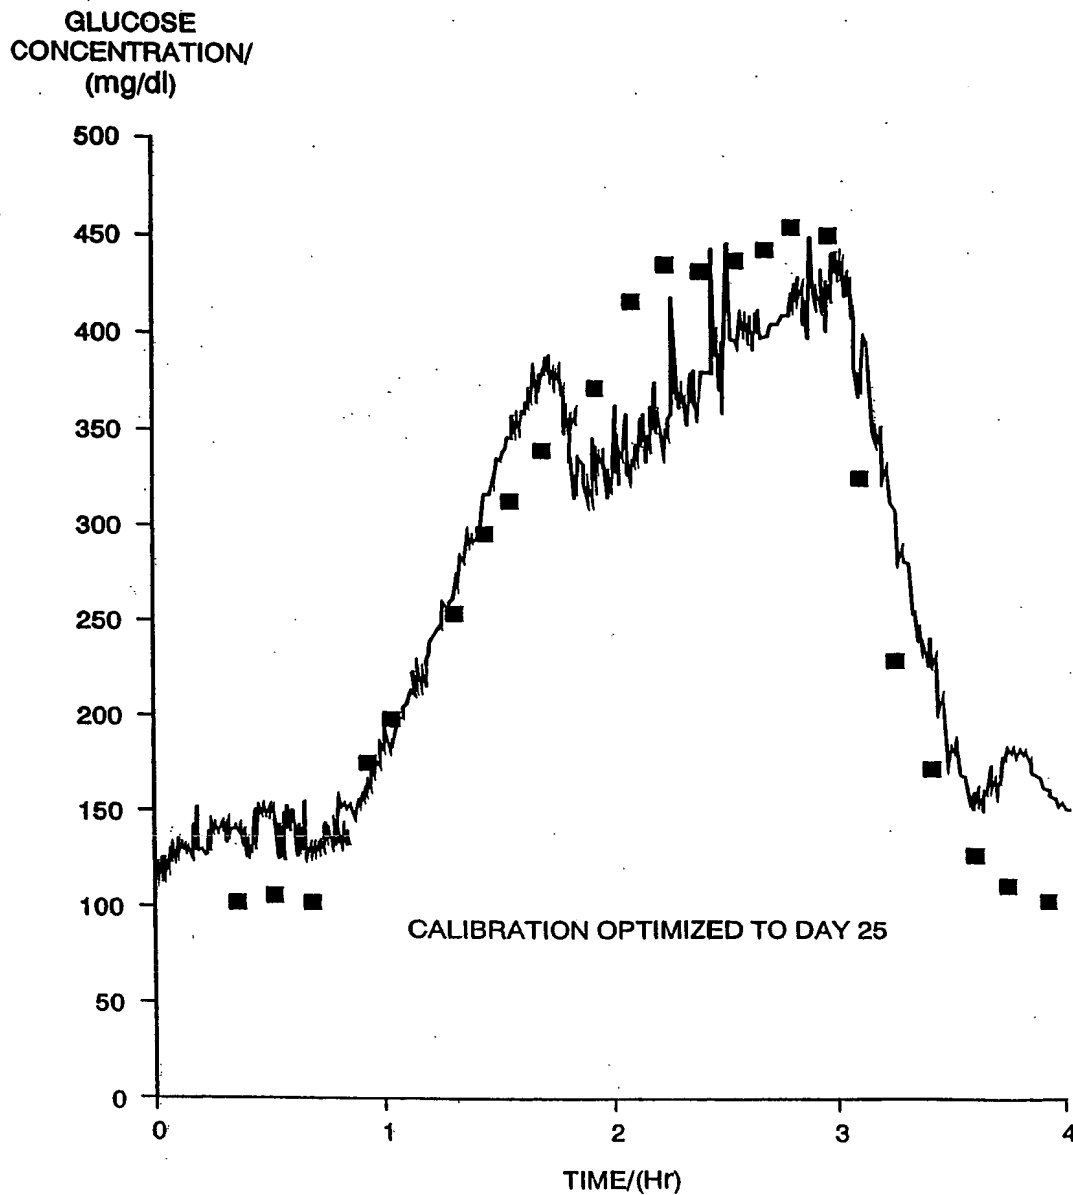


FIG. 5A



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588

Atty Docket: DEXCOM.8DVC1

8/10

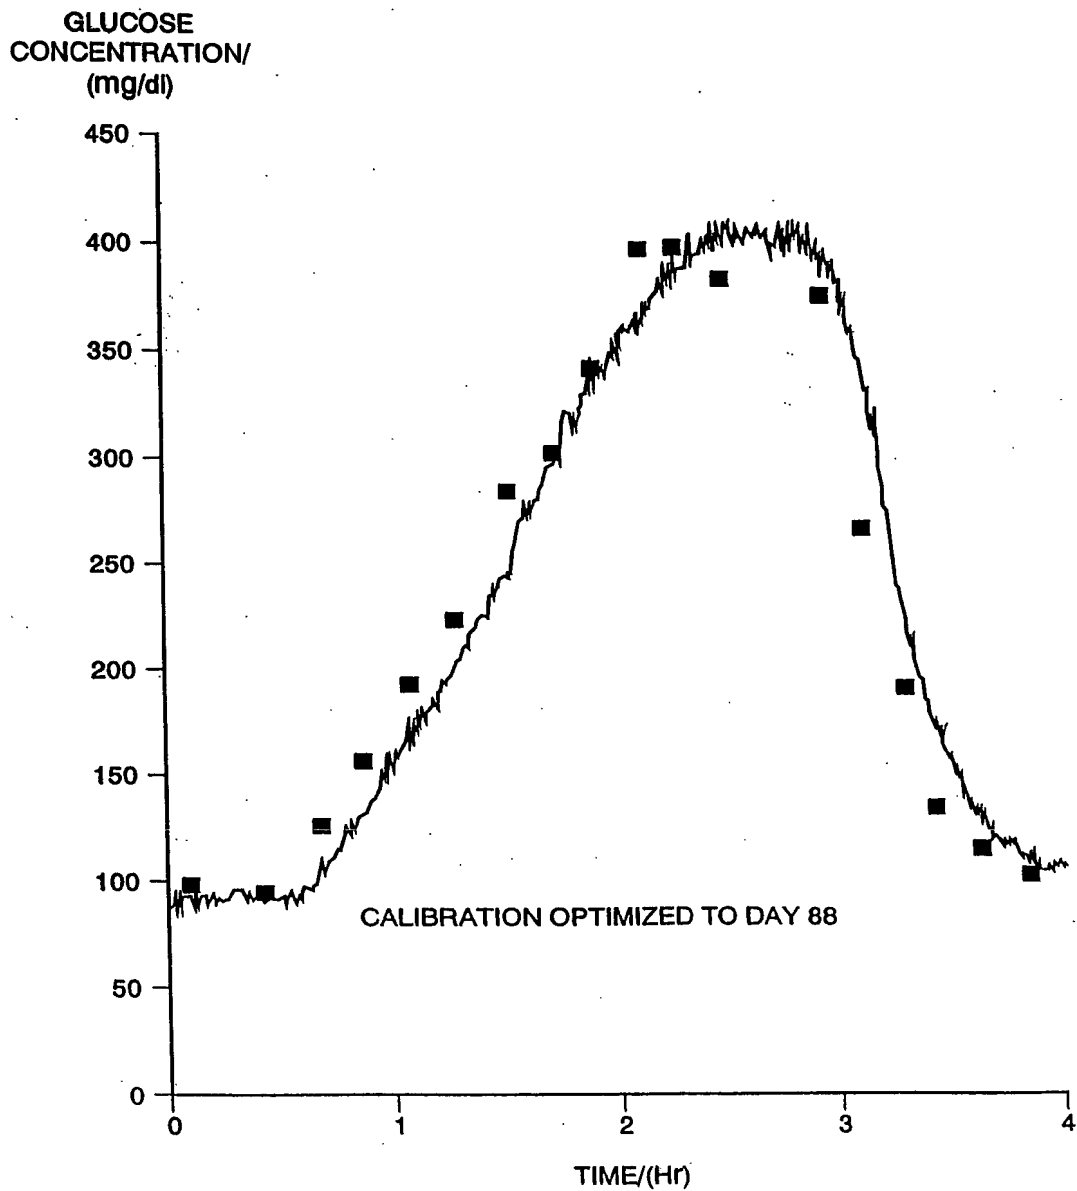


FIG. 5B



9/10

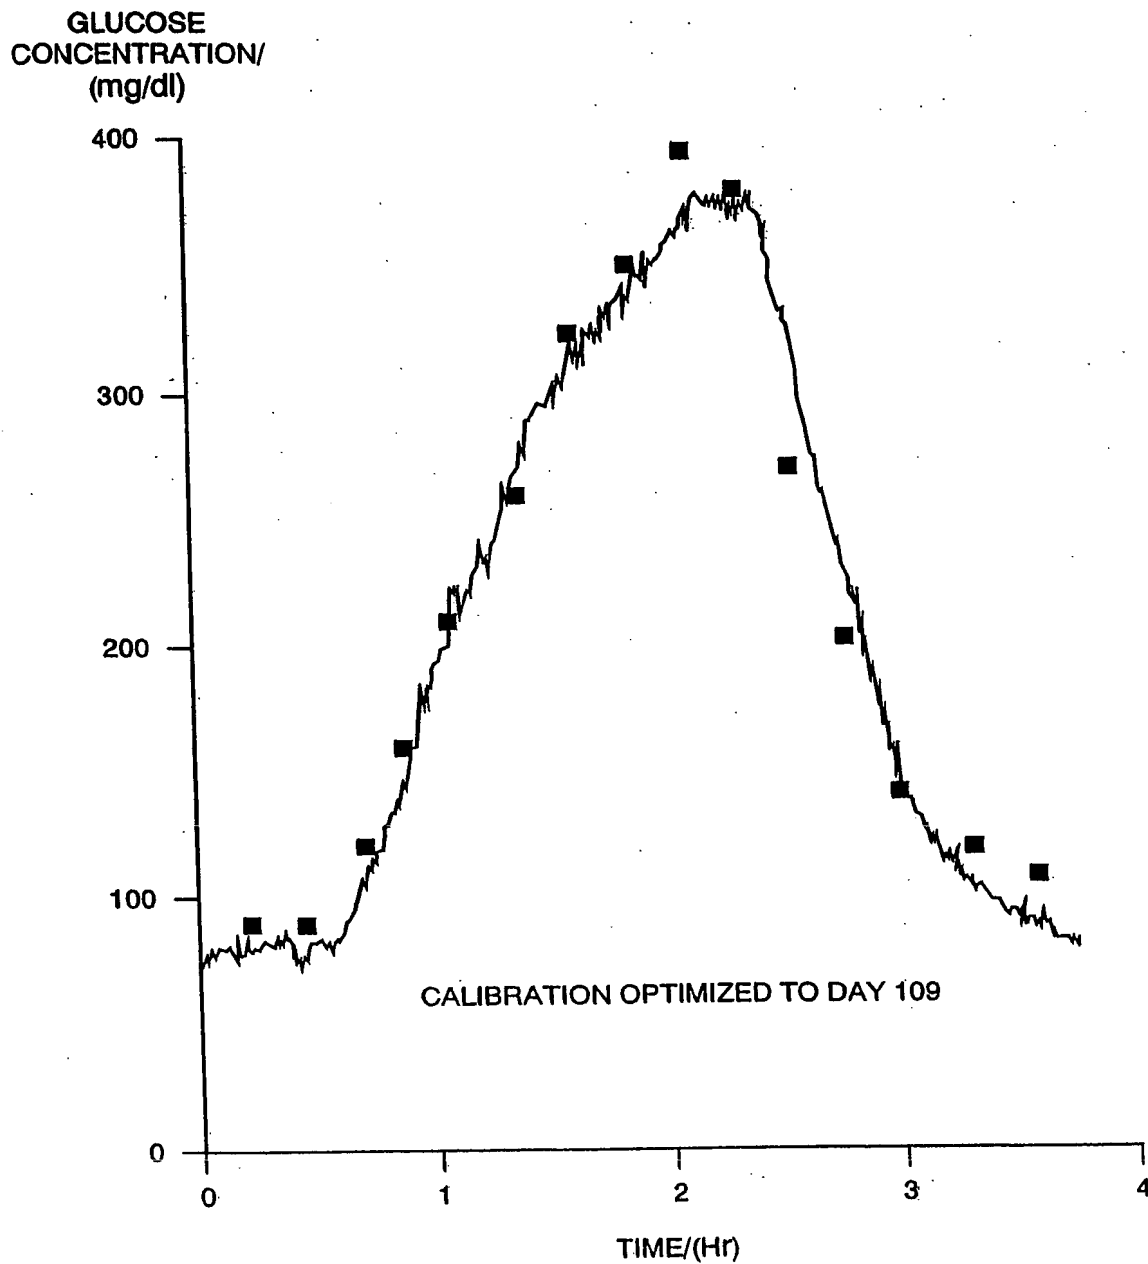


FIG. 5C



DEVICE AND METHOD FOR DETERMINING ANALYTE LEVELS

Shults, et al.

Appl. No.: 09/489,588

Atty Docket: DEXCOM.8DVC1

10/10

SENSOR
GLUCOSE/
(mg/dl)

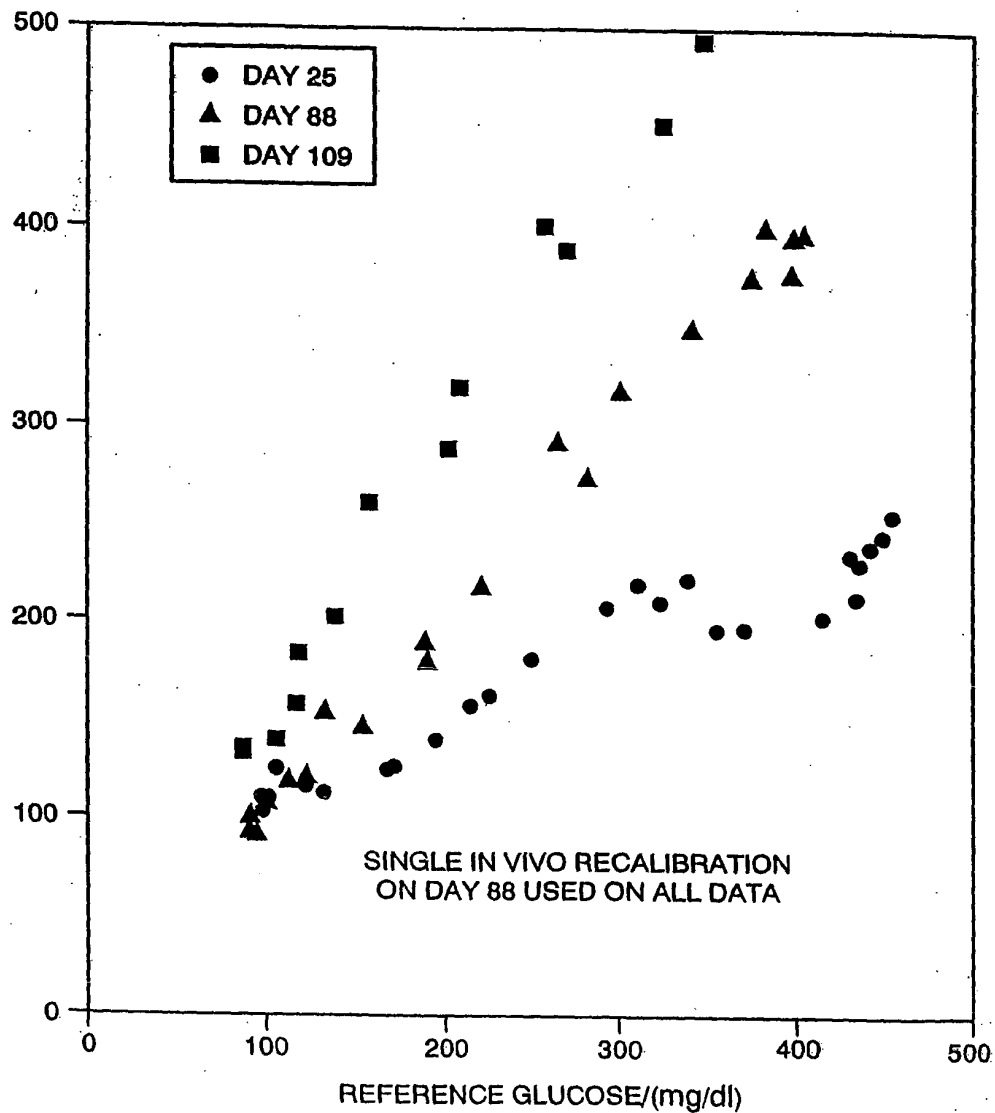


FIG. 6